



### Instruction of exchanging the round belt in MD-10 XRD




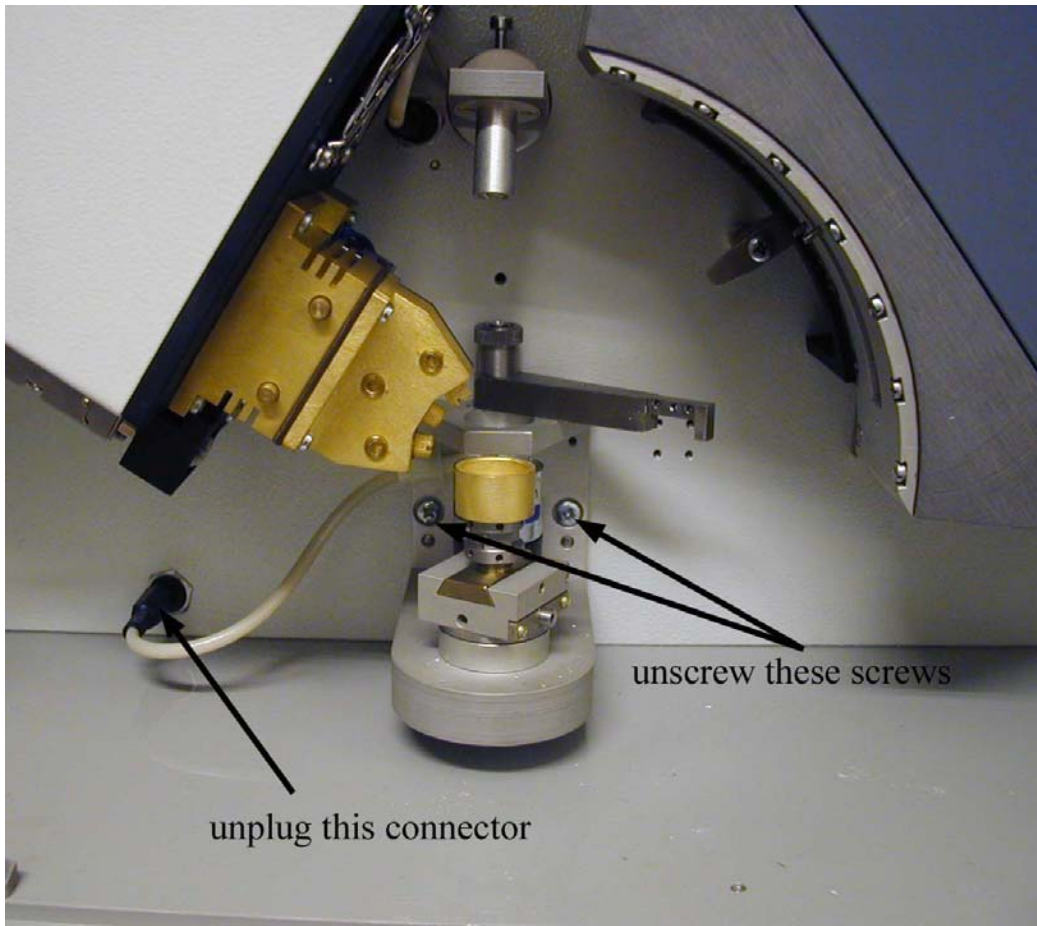

Unscrew the holder and pull off it.  
Sample holder

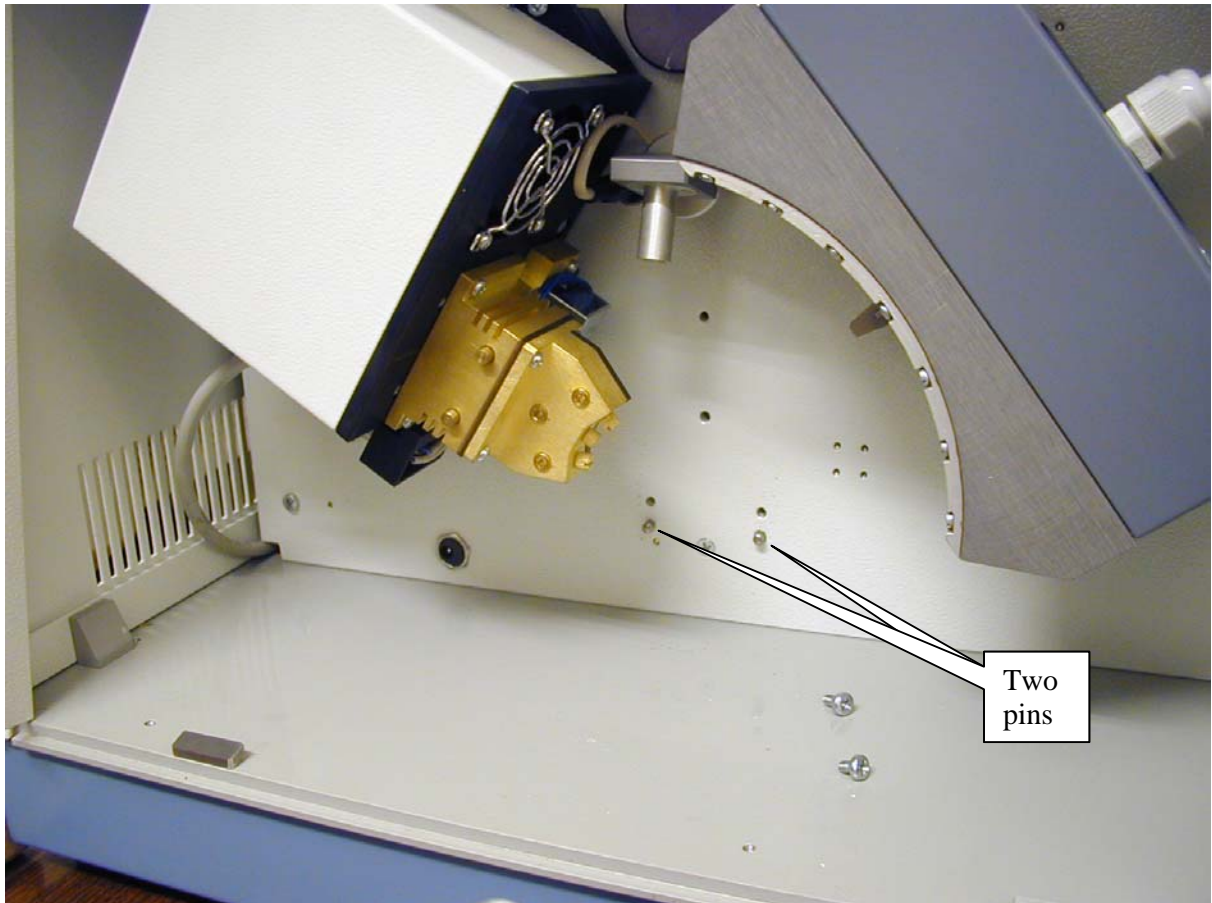

The holder is located on two pins and when you will place it back; these pins ensure the previous position of the holder. It is no need to align the holder. It will be necessary to calibrate the diffractometer after that.

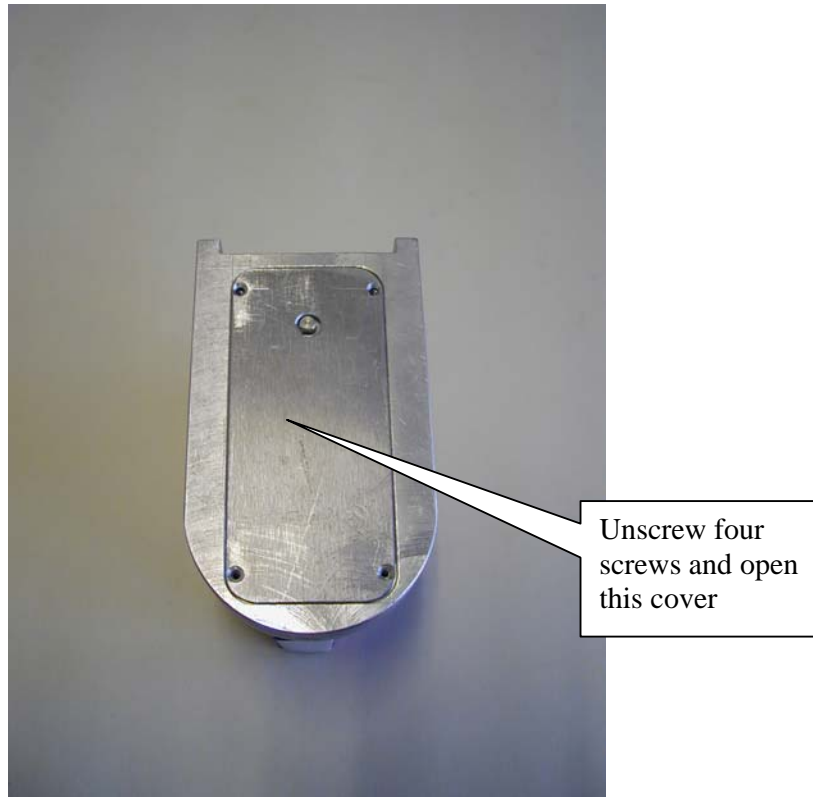

Bottom view of the sample holder  
Open the bottom cover of the holder. Two pulleys should be connected by the round belt. It is necessary to replace this round belt.